


LEAP X-Press

Filtration Just-In-Time, for LC or GC



- UniPrep™ Automated

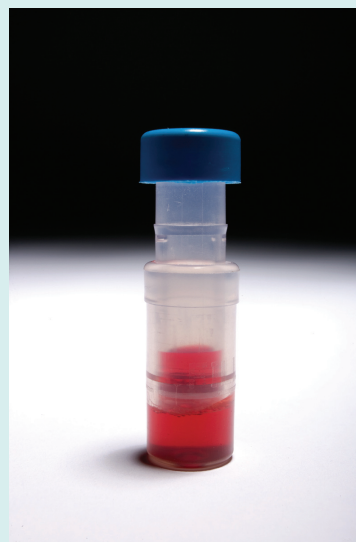

- Protect Your LC-Column
- Protect Valuable Samples
- Replace Syringe Filters
- Electric Motor with Innovative Torque Limit
- No Rupturing of Filter Seal

- Filtration for UHPLC, Plant Extracts, and Many Other Dirty Samples
- Use Any Filter Media with Mini-Uniprep
- Fast and Consistent Filtration


Complete Automation from Sample Vial to Recovering Filtrate



www.leapte.com • info@leapte.com • www.leapwiki.com
Tel 800-229-8814 • 919-929-8814 • Fax 919-929-8956

LEAP X-Press

Automated Sample Filtration

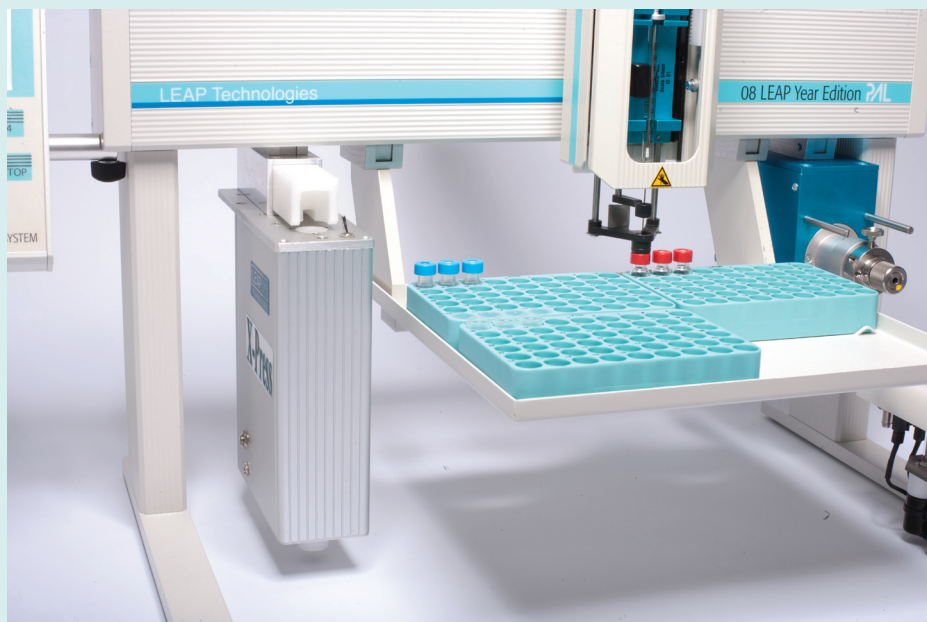

Filtration on a Single Disposable: For a Large Variety of Situations

- Samples before injection onto an UHPLC system
- Any solution with particles
- Plant extracts

- **Stand-Alone with optional switch for semi-automated mode**

or

- **Fully automated as an accessory on a CTC PAL**



The raw samples can be placed in microtiter plates or vial racks. The PAL injector head completes the whole workflow in less than 2 minutes, with the capacity limited only by the rack space on the PAL